



1/9

Figure 1

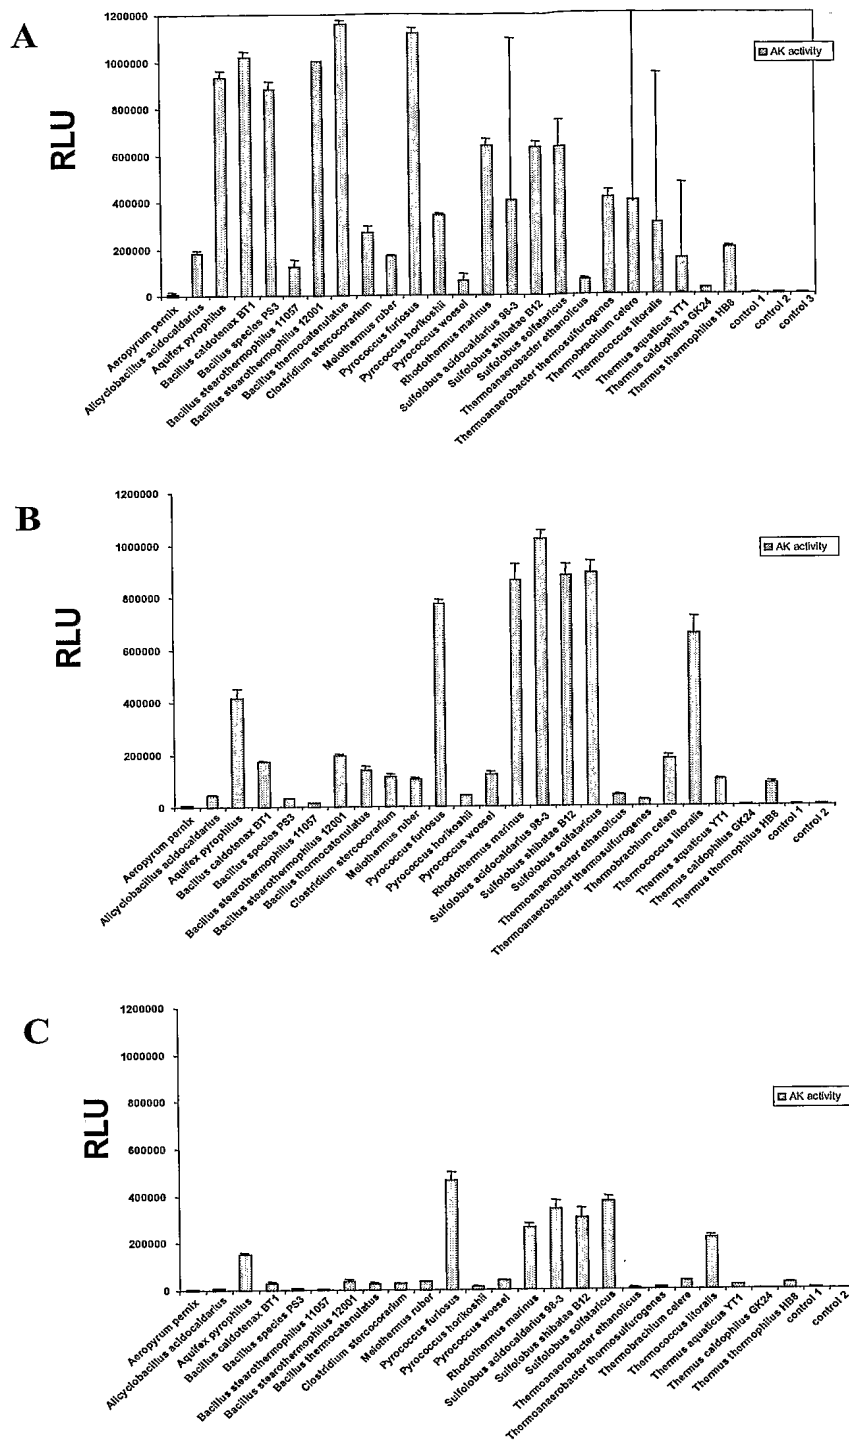




2/9
Figure 2

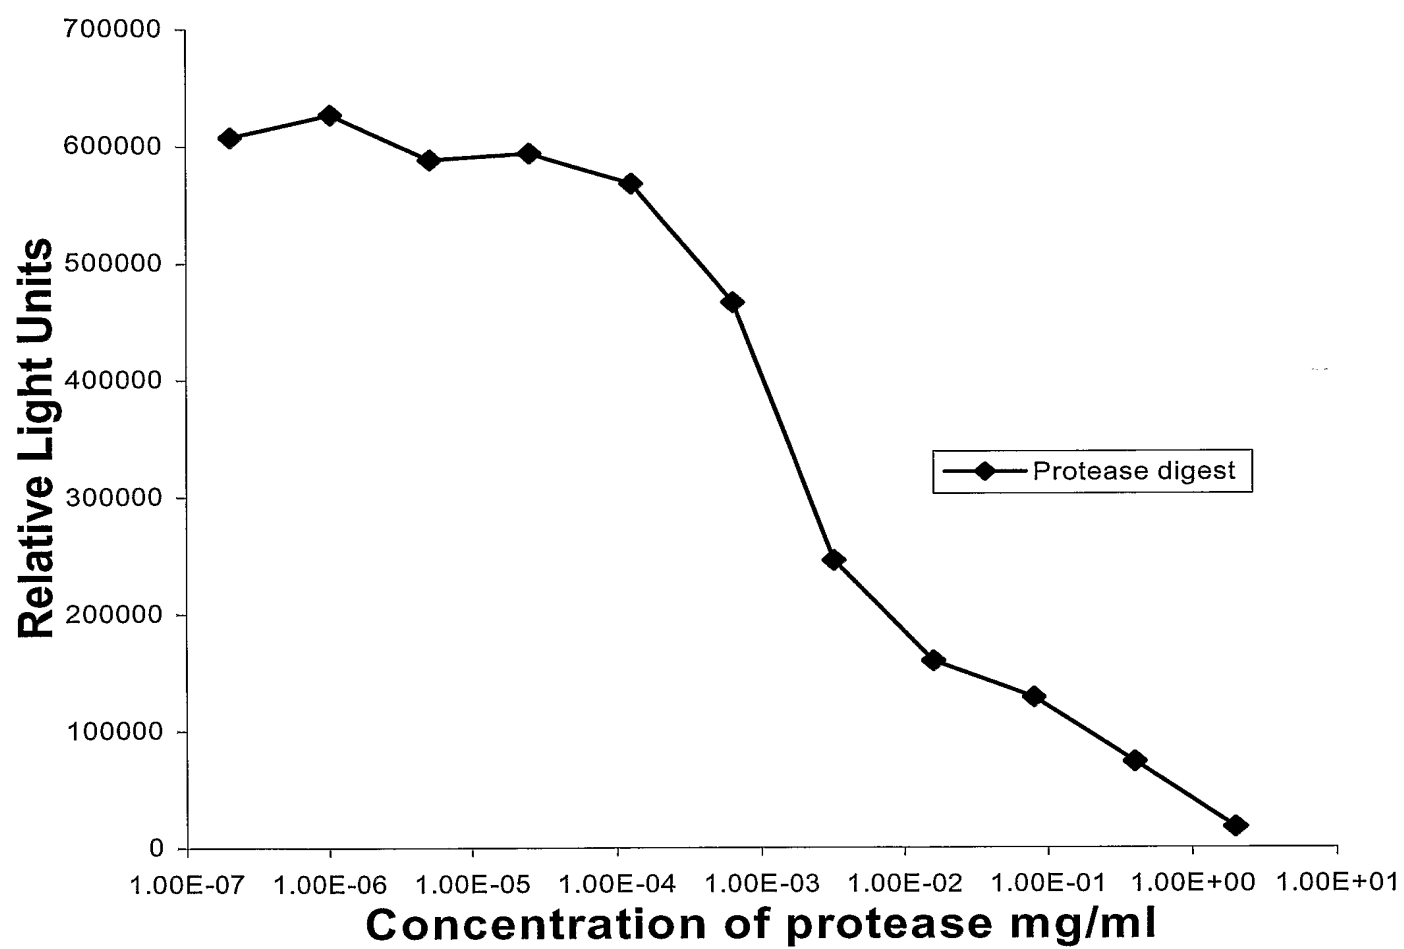


3/9
Figure 3

Dynamic range of adenylate kinase indicator with varying temperature

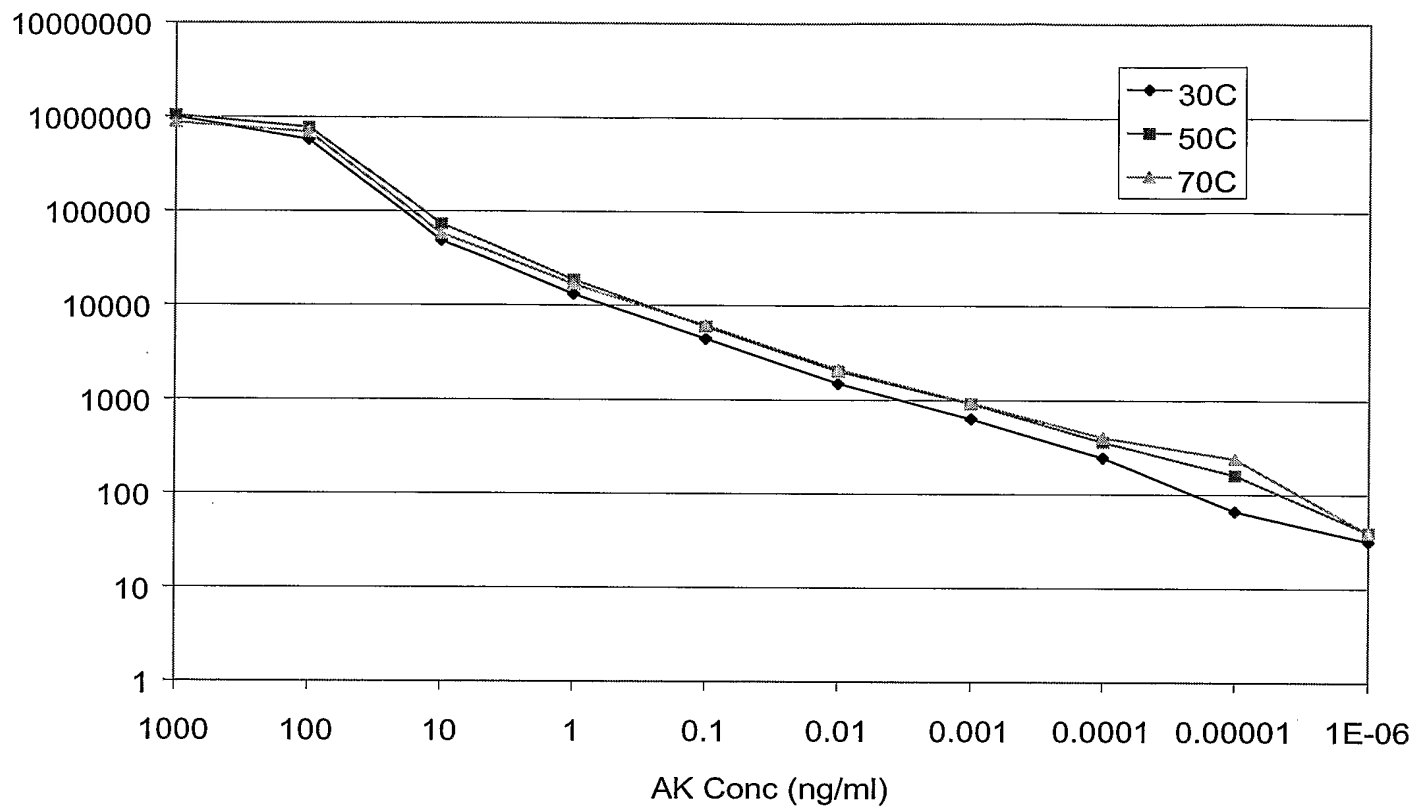

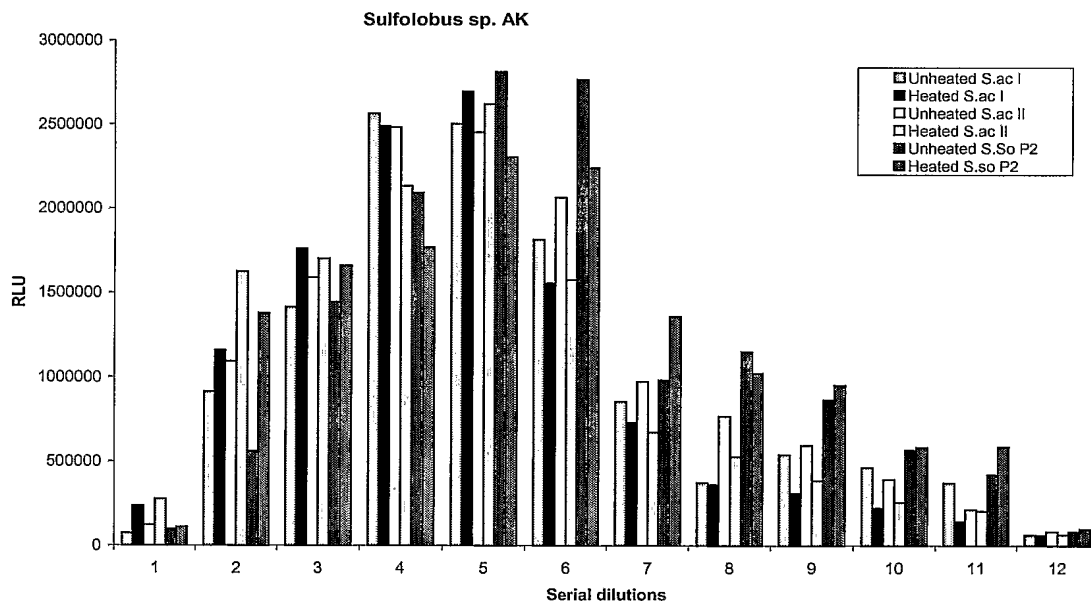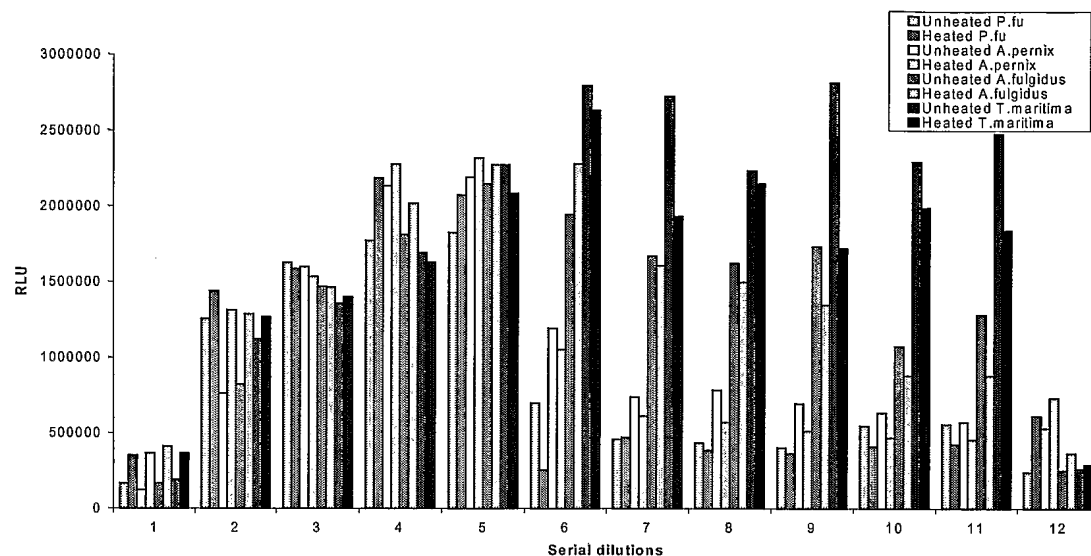
4/9
Figure 4

5/9
Figure 5

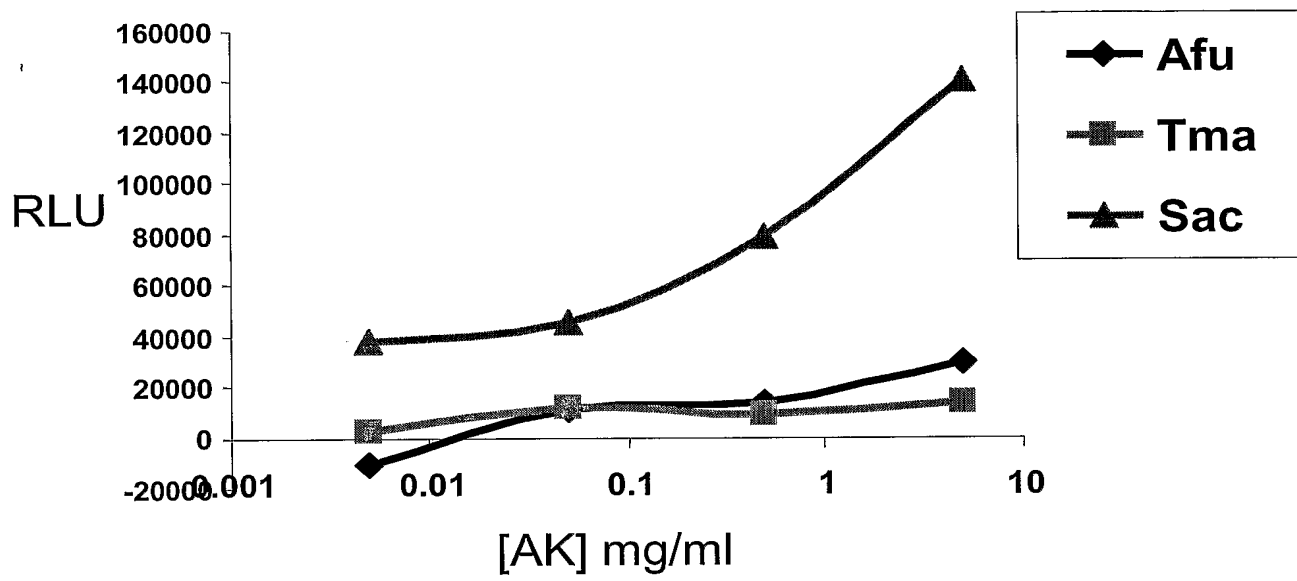


6/9
Figure 6

A.

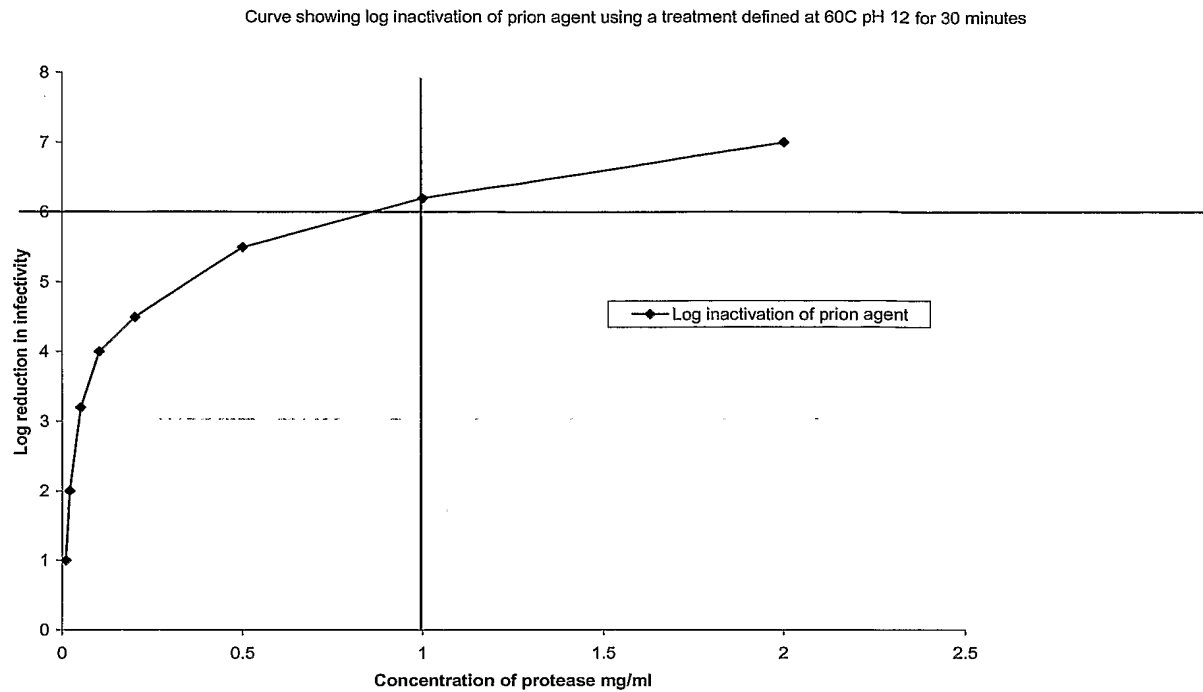


B

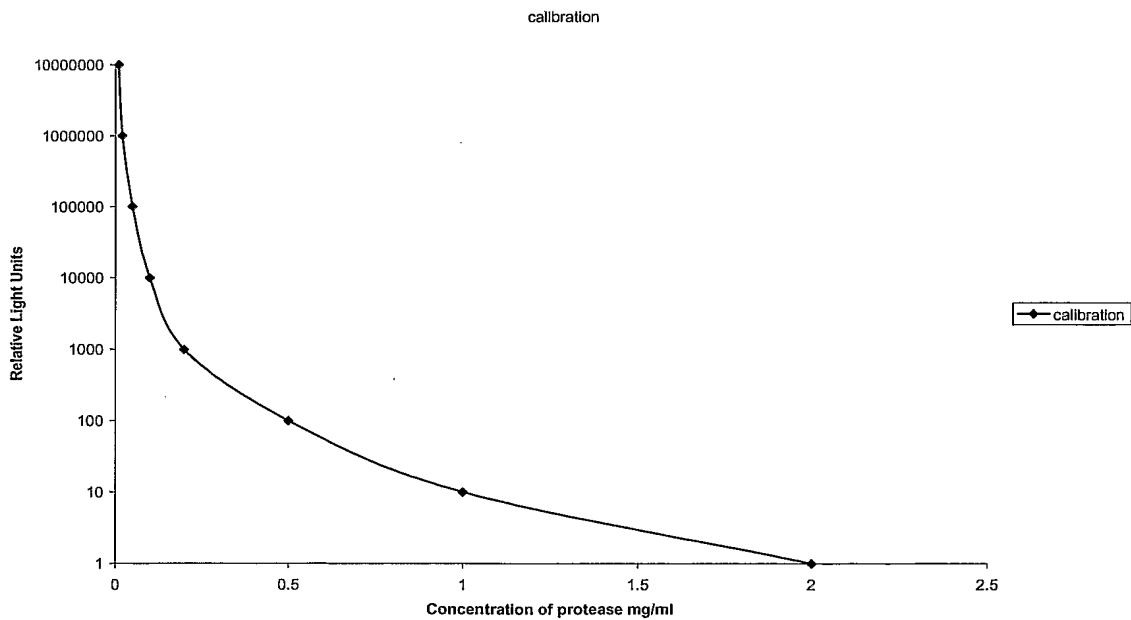


7/9
Figure 7

A.

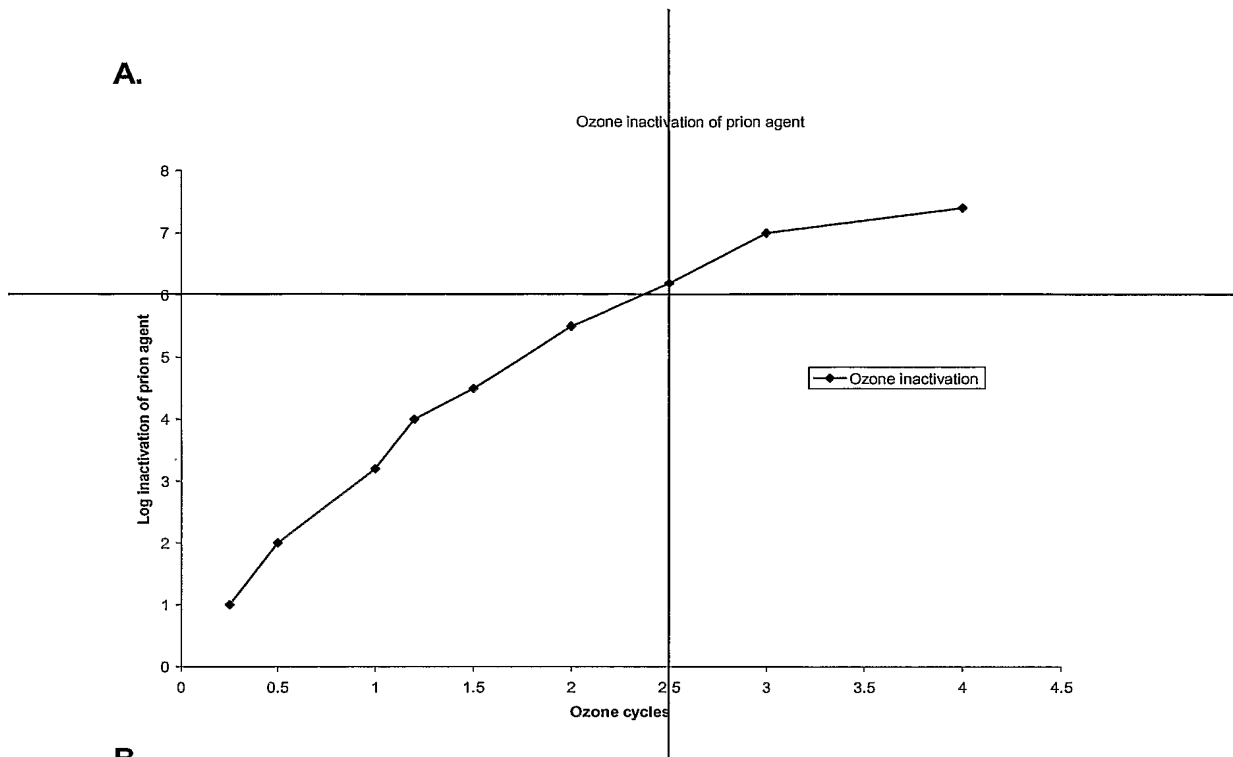


B.

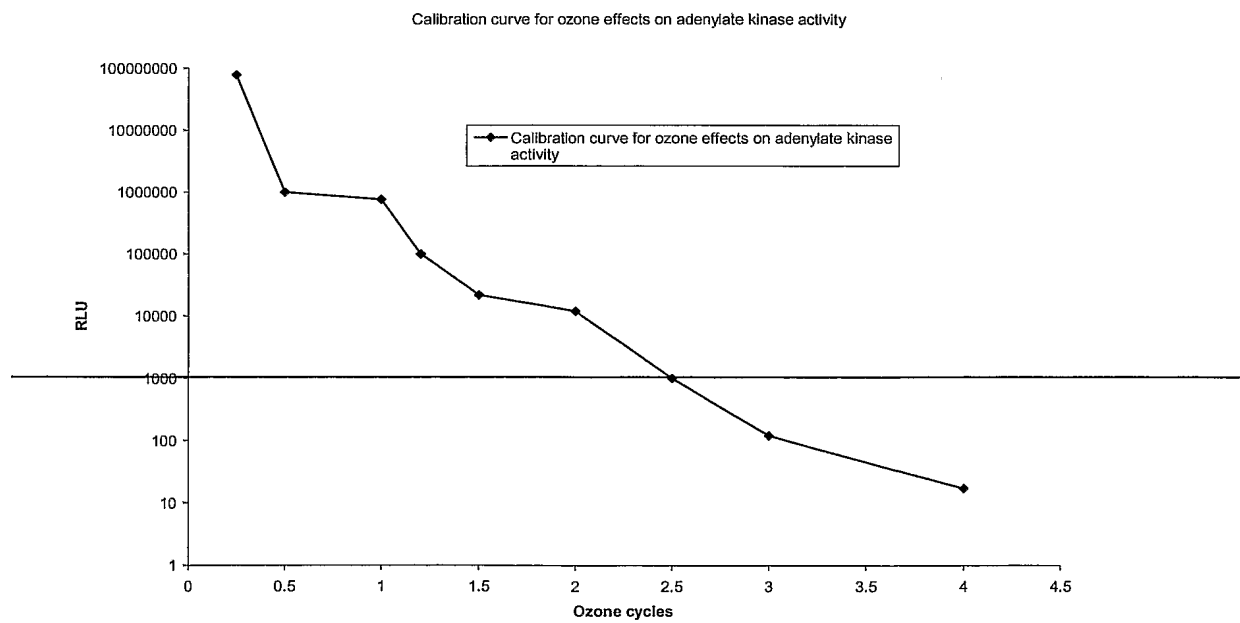

8/9
Figure 8

A.

Removal of standard soil within a washer-disinfector with Formulation X

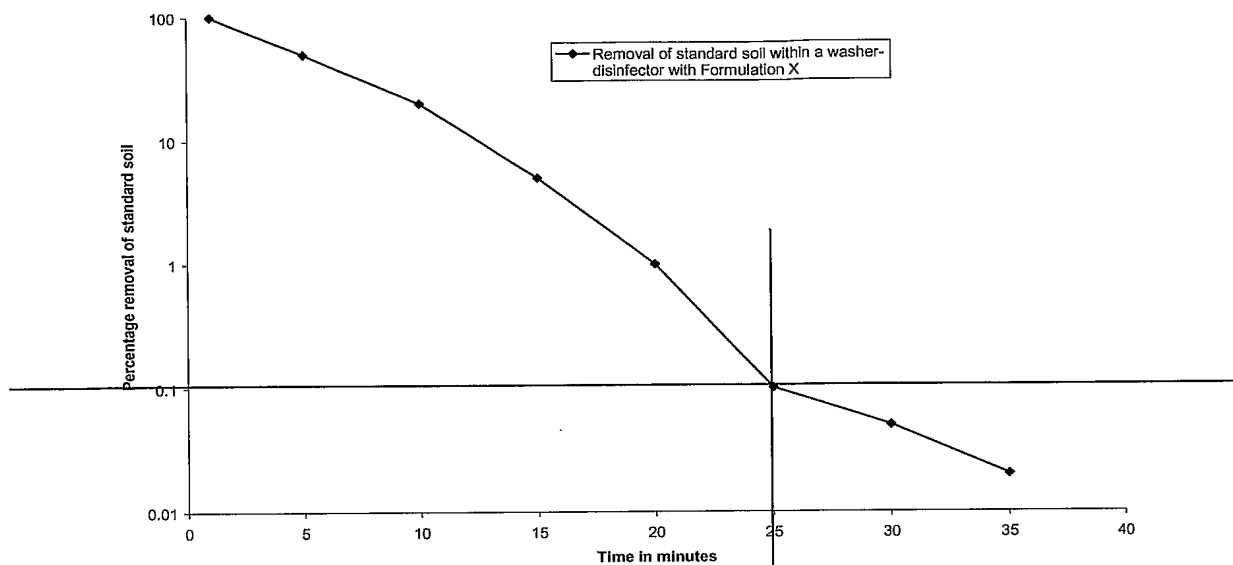

B.

Calibration curve for washer disinfector indicator

